

MEASUREMENT PROTOCOL

No. PM_TTP_OPT_RR_MM_DD_XX

Order number 123456
Customer ZČU, TTP


Sample label customer S123456
 NTC 210417-002

Measured quantity effective directional emissivity
Measurement method EDEHT
Detection system FLIR A615
Temperature (T) 100 to 900°C, temperature step 100°C
Viewing angle (θ) 20°

Date 17.4.2021

Measured by Ing. Matěj Hruška

Responsible person Ing. Petra Honnerová, Ph.D. Phone: +420 377 634 719
 Email: petrahon@ntc.zcu.cz

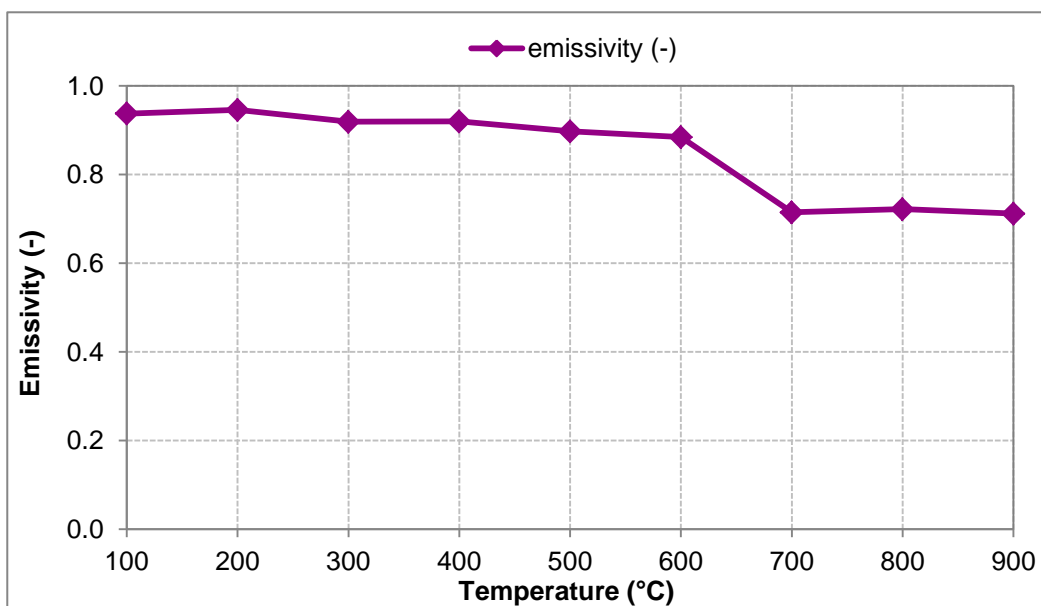

temp. (°C)	100	200	300	400	500	600	700	800	900
emissivity (-)	0.938	0.946	0.919	0.920	0.898	0.884	0.715	0.722	0.712