

MEASUREMENT PROTOCOL

No. PM_TTP_OPT_RR_MM_DD_XX

Order number 123456

Customer ZČU, TTP

Sample label customer S123456
NTC 200904-001/001

Measured quantity spectral normal emissivity

Measurement method SNEHT


Temperature (T) 900°C

Polar angle 0°

Date 30.3.2021

Measured by Ilona Slavíková

Responsible person Ing. Petra Honnerová, Ph.D. Phone: +420 377 634 719
Email: petrahon@ntc.zcu.cz

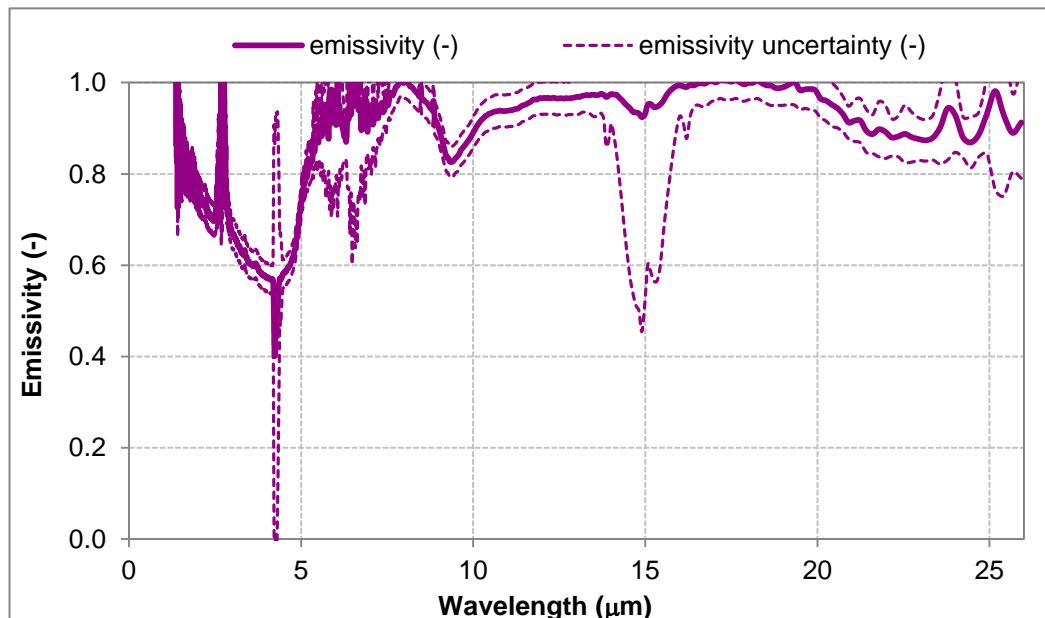

WL (um)	2	3.5	4.7	8.3	10	12.5	17.5	20	25
emissivity (-)	0.765	0.605	0.605	0.982	0.892	0.966	1.002	0.983	0.932
un. (-), k = 2	0.034	0.032	0.031	0.036	0.034	0.036	0.041	0.046	0.049